

User manual
JOFRA STS-050 A/B
Probes 250/350/500/901

© Copyright 2006 AMETEK DENMARK A/S



Visit **TRANSCAT**.com >

sales@transcat.com | 800.828.1470

Table of contents:	Page
1.0 General information	4
2.0 Introduction.....	5
3.0 Functionality	6
3.1 Functional description	6
3.2 Connections	6
3.3 Serial number	8
4.0 Operation	9
4.1 Operation area	9
5.0 Maintenance.....	10
6.0 Technical specifications	11

1.0 General information

This manual is only effective for the following products:

JOFRA STS-050 A/B - 250 mm

JOFRA STS-050 A/B - 350 mm

JOFRA STS-050 A/B - 500 mm

JOFRA STS-050 B - 901 (90°)

The products are manufactured by:

AMETEK DENMARK A/S
GYDEVANG 32-34
DK-3450 ALLERØD
DENMARK
TEL: +45 48 16 80 00
FAX: +45 48 16 80 80

2.0 Introduction

The JOFRA STS-050 A/B probes are designed for fast and traceable calibration and temperature measuring with AMETEK DTI050, and are ready for use.

Please read this manual carefully before use, to obtain maximum value of your calibration system.



Warning

- Read this manual before use.
- Do not use in hazardous area.
- Handle carefully.
- Never exceed temperature range

3.0 Functionality

3.1 Functional description

The probe can be used for measuring temperature in the range -50°C to 400°C (-58°F to 752°F).

The JOFRA STS-050 A/B probes may be supplied with certificates for a limited temperature range.


The resistance of the JOFRA STS-050 A/B probe is converted to temperature according to IEC-751 (ITS-90) (calculated coefficients specific for the probe is stated on the certificate).

3.2 Connections

The probe is delivered with a connecting cable.
The pin-layout is as follows:


- Pin 1 : RTD I-/ CJC Pt1000 –
- Pin 2 : RTD S-/ TC V-
- Pin 3 : RTD S+/ TC V+
- Pin 4 : RTD I+/ CJC Pt1000 +
- Pin 5 : Memory GND
- Pin 6 : Memory I/O

The figure below is shown from the connector side of the probe connector.

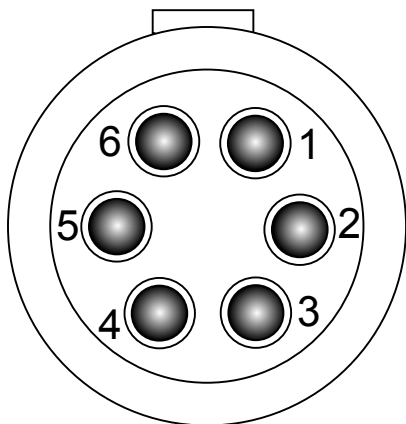

3.3 Serial number

The serial number is placed on the probe as shown on the figure below:

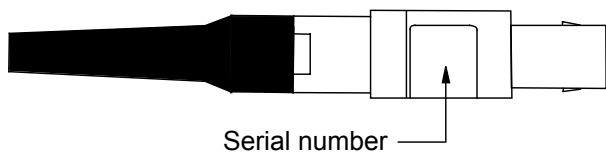

4.0 Operation

4.1 Operation area

All the probes are intended for use in areas which meet the following:

Ambient temperature

range : -20°C to 70°C (-4°F to 158°F)

Humidity : 0% to 90%

Protection class : IP 50



Warning

Do not use in hazardous areas.

5.0 Maintenance

The probe does not require specific maintenance before or after use. The user may carry out the following procedure himself:

- Cleaning the probe : Use alcohol or water and a soft cloth.



Caution...

- The probe must always be protected against any mechanical damage.
- The probe must never be exposed to mechanical shock effects.
- Avoid thermal shock
- Any bending of the probe may cause permanent damage

6.0 Technical specifications

Probe specifications:

Sensor type	:	Platinum sensor Pt100. $\alpha = 0.00385$
Probe length	:	250 mm (9.8 in) 350 mm (13.8 in) 500 mm (19.7 in) 180 mm (7.1 in) (90° Angle)
Temperature range	:	-50°C to 400°C (-58°F to 752°F)
Accuracy		
Repeatability	:	0.005°C (0.009°F)
Hysteresis ¹⁾	:	0.01°C @ 0°C (0.02°F@32°C)
Stability ²⁾	:	typ. 0.014°C @ 0°C (0.025°F@32°F)
Self heating effect	:	0.04°C/mW / 0.07°F/mW
Diameter	:	A: OD4 mm B: OD1/4"
Immersion depth	:	A: 60 mm (2.36 in) B: 90 mm (3.54 in)
Media compatibility	:	AISI316

1)When used in the range -50°C to 400°C (-58°F to 752°F)

2) Stability when exposed to 400°C (752°F) for 100 hours.
Stability will depend on actual use of the probe.

Response time : A: $\tau(50\%) = 7 \text{ sec.}$
 $\tau(90\%) = 17 \text{ sec.}$

B: $\tau(50\%) = 11 \text{ sec.}$
 $\tau(90\%) = 30 \text{ sec.}$

Recommended
meas. current : 1 mA

Connection : Redel plug with build in
memory is standard

Certificate:

All probes are supplied with an traceable certificate according to the ITS 90 temperature scale. The probes are as standard calibrated in the range – 45°C to 400°C (-49°F to 752°F).

Calibration is carried out at:

- -45°C/-49°F
- -20°C/-4°F
- 0°C/32°F
- 100°C/212°F
- 250°C/482°F
- 400°C/752°F

Visit **TRANSCAT**.com >

sales@transcat.com | 800.828.1470